

LUXTEC®



MLX 300 WATT XENON LIGHT SOURCE Operation and Service Manual ENGLISH

99 Hartwell Street
West Boylston, MA 01583 USA
Tel: +1-508-835-9700
US Toll Free: 1-800-325-8966
Fax: +1-508-835-9976
Website: <http://www.integra-surgical.com>
E-mail: custsvcluxtec@integra-surgical.com

TABLE OF CONTENTS

PAGE	DESCRIPTION
2	Indication For Use
3	Symbols
4	General Warnings
4	Precautions
5	Overview
5-6	Operation
6-7	Xenon Lamp Module Replacement
8	Fuse Replacement
9	Optional Floor Stand Assembly
10	Replacement Parts and Accessories
10	Maintenance and Cleaning
11	Troubleshooting
12	Specifications
13-15	Electromagnetic Compatibility (EMC) User Information
16	Block Diagram
17	Repair and Return
17	Limited Warranty


INDICATION FOR USE

The Luxtec MLX light source is designed to supply high-intensity white light to a fiber optic cable for illumination of a surgical field during a surgical and/or medical procedure.

SYMBOLS

TABLE OF SYMBOLS

Found on a medical grade light source, other illumination related equipment, fiber optic cables and corresponding packaging.

	Attention; Consult Accompanying Documents		Fuse
	Caution: High Voltage		Type CF Equipment
	Equipotentiality		Type BF Equipment
	Protective Earth		High Temperature
	On / Off		Brightness
	Stand-by		Motor
	System Status Display		Fan
	System		CE
	Do Not Dispose		Listed by ETL
	Push		Listed by CSA
	Hours		Part Number
	Over Temperature		Batch Code
	Intensity		Serial Number
or 	Lamp		Authorized Representative in the European Community
	Keep dry		Manufacturer

GENERAL WARNINGS

- The user should carefully study the Operation and Service Manual before using the equipment in a clinical environment. Instructions should be followed, with special attention given to warnings, controls and user specifications. The Manual should be available to the appropriate personnel.
- This Manual contains information about the proper procedures for preparing this product for its use and care.
- Before every procedure, carefully inspect the light source to ensure it has been properly maintained and cleaned, and that it is fully functional. **DO NOT** use if inspection reveals any damage such as case damage or loose connectors.
- Follow the instructions of other manufacturer's equipment when used in conjunction with this product.
- To reduce the risk of fire and electric shock, do not expose electrical equipment to moisture. When cleaning, do not immerse any electrical device in liquid.
- Do not use or store liquids on or above the light source.
- **SAFETY PRECAUTIONS MUST ALWAYS BE EXERCISED WHEN USING ELECTRICAL EQUIPMENT TO PREVENT OPERATOR/PATIENT SHOCK, FIRE HAZARD OR EQUIPMENT DAMAGE.**
- Electric shock hazard. If unit is not functioning properly, **DO NOT OPEN**. Please refer to the Repair and Return Section of this Manual.
- All electrical equipment must be used with approved hospital grade power cords and power plugs inserted properly into grounded AC power outlets.
- The light source should never be used in ocular surgery or in a surgical procedure requiring direct illumination of the eye.
- Use care not to point any fiber optic cable directly at the eye while operating the light source.
- The light source produces high intensity light. Thermal burns can result from improper use of the light source or from the light output of the fiber optic cable.
- Explosion Hazard. Do not use in the presence of flammable anesthetics, liquids, vapors, gases or dusts.
- Keep cooling vent and fans free of obstructions.
- **FIRE HAZARD: DO NOT DRAPE OR COVER THE LIGHT SOURCE WHILE IT IS OPERATING.**
- When light source is not in use, turn off the power or put the unit in stand-by mode.
- Ensure that the fiber optic cable matches the port type to prevent damaging the optical components of the light source. For user convenience, the light source has a turret with labeled selectable ports.
- Do not use the headlight at distances of less than 10" (25cm).

PRECAUTIONS

- Take precautions to verify that the fiber optic cable is appropriately suited for the light source. Xenon and other high illumination light sources require premium fiber optic cables in order to achieve optimal performance and prevent damage to the fibers, thereby diminishing the quality of the light output or the useful life of fiber optic cable.
- Take precautions not to touch or disconnect the cable end fitting from the turret until the Light Source has been "shut down" for a period of time and allowed to cool. The cable end fitting will remain hot immediately following shut down, which can cause burns.
- Take precautions to not place and rest a hot cable end fitting and/or head light on a patient or allow the system to come in contact with un-protected hands or tissue. The entire system should be allowed to cool following use. Failure to do so can cause burns and/or tissue damage.

OVERVIEW

The MLX light source delivers 300 spare watts of cool white infrared (IR) filtered light. The lamp is housed in a lamp module that can be easily serviced without special tools.

Set Up and Inspection Before Use

The light source comes with the hospital grade power cord packaged separately. Verify that both components are in good condition.

Before turning power on to the light source, make sure the unit is plugged into any standard 100VAC to 240VAC 47-63Hz (as appropriate) outlet. Grounding reliability is guaranteed only when connected to a “hospital grade” receptacle.

Allow a minimum of 2 inches (5.08 cm) clearance at the rear and sides of the unit for cooling air flow. Ensure that the unit is not near air exhaust or against other equipment.

WARNING: The MLX light source monitors air intake temperature and will turn off if ambient temperature is $> 40^{\circ}\text{C}$

OPERATION

1. Insert a fiber optic cable in the proper port in the turret. The active port is indicated by a on (See Figure 1). Available ports are ACMI, Olympus, Storz and Wolf cable-compatible. All ports are identified appropriately.
2. Press the Power Switch in the upper left corner of the front panel (See Figure 2).
3. When the Power Switch is pressed the Stand-by Light (Figure 2) will blink and there will be a 3 – 4 second delay before the Xenon Lamp illuminates while the system does a self-diagnostic check.
4. Press the Stand-by Button.



Figure 1

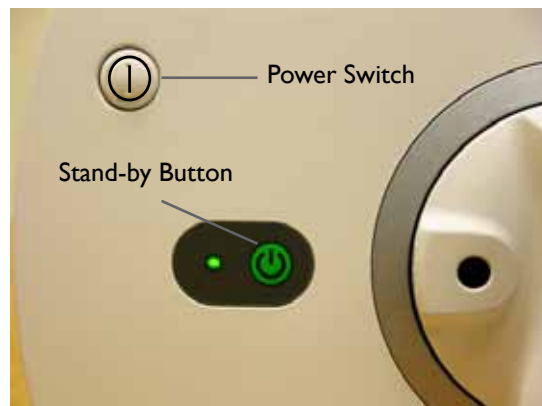


Figure 2

OPERATION

5. The system will start up at the same light intensity as when last used (Figure 3). For new systems, the light intensity will start at the minimum 20% setting.
6. To adjust the light intensity, push the Membrane Switches (Figure 3): + to increase or - to decrease the light output or intensity. Range is 0%, 20 – 100% in 5% increments. Holding the + or – button will change the intensity more quickly.

NOTE: It is strongly recommended that the light be used at the minimum intensity for good visualization.

7. The System Status Display can be pressed to show both lamp time and system operation time. A second press of the switch will show the software version of the system monitor. A third press returns to light output. (The system will automatically return to the light intensity reading after 15 seconds).

8. The system can be placed in stand-by mode (no light emitted) allowing the surgeon to unplug a headlight and move around the table, or to change cables in a laparoscopic or endoscopic procedure.

CAUTION: Cable end fitting can be HOT!!!

NOTE: If unit is left in stand-by mode for 15 minutes, it will automatically shut off the lamp. Fans will keep running. To re-activate, push the Stand-by Button.

9. To shut the system off, simply press the main Power Switch as in Step 2.



Figure 3

XENON LAMP MODULE REPLACEMENT

Note: Please adhere to appropriate safety precautions when performing lamp replacement. Only qualified personnel should service this device. Protective facemask and/or proper safety glasses should be worn when replacing the lamp module. Before changing the lamp module, turn power off and allow the light source to cool for at least fifteen (15) minutes.

Please read and comply with all Precautions and General Warnings listed in this manual.

XENON LAMP MODULE REPLACEMENT

To remove:

1. Make sure the power is off and the hospital grade power cord is disconnected.
2. Remove the retaining screws from the top plate (Figure 4) and retain screws.
3. Slide the top plate towards the back of the unit until it stops.
4. Lift the top cover up and off the unit.
5. Unscrew the lamp module door and remove (Figure 5) and retain screw.
6. Grasp the module by the tabs and pull directly up (Figure 6).



Figure 4



Figure 5

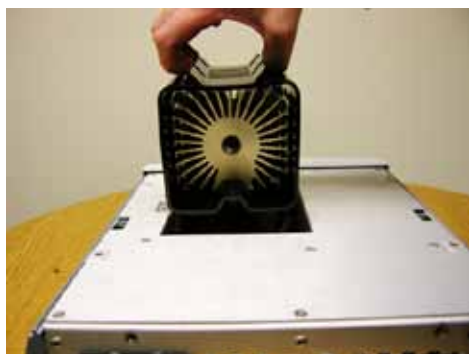


Figure 6

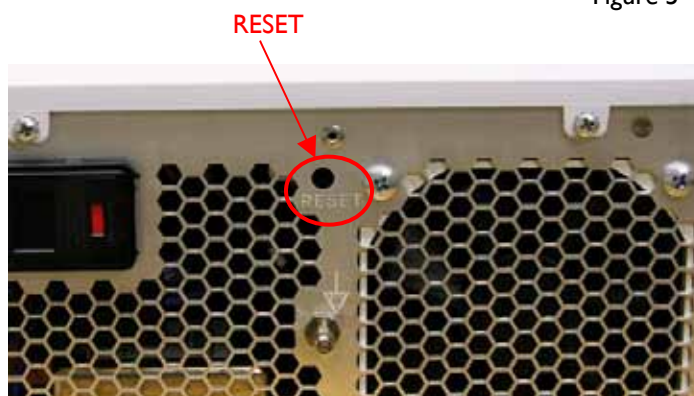


Figure 7

To Replace:

1. Orient the lamp module (P/N 001320LX) to face forward.
2. Place the module into the light source.
3. Seat module securely.
4. Replace the lamp module door and secure it with the screw.
5. Align top cover brackets into slots and slide forward.
6. Slide the top plate forward until it engages the front panel.
7. Replace the retaining screws in the rear panel.
8. Replace the hospital grade power cord and turn on power to verify operation.

To Reset Lamp Age Meter:

1. Using the membrane switch, turn the display to the lamp age/system age screen.
2. On the rear of the unit insert a pen/pencil or other suitable pointed object into the slot marked RESET (Figure 7).
3. Push until a click is felt.
4. Verify that the lamp age has been reset to 0.

NOTE: The System Age reading **CANNOT** be reset.

FUSE REPLACEMENT

To replace the fuse:

- The fuse for the light source is located in the power entry module in the rear of the unit.
- Remove the hospital grade power cord from the back of the light source.
- Using a small flat screwdriver, pry open the retaining door (Figure 8) and pry out the red plastic block from the power entry module (Figure 9).
- Check to see if the fuse is blown; if blown replace with a fuse of the same rating (Luxtec P/N 600987, or T6.3AL250).
- Replace the red block in the housing.
- Snap the retaining door into place.
- Plug cord back into light source and retest the unit.



Figure 8



Figure 9


OPTIONAL FLOOR STAND ASSEMBLY

There are four (4) parts to the floor stand assembly:
(Figure 10).
(Phillips head screwdriver included for assembly)

1. Base with five (5) casters (2 locking)
2. One column with light source base plate
3. Handle
4. MLX light source base

Floor stand assembly instructions:

1. With the handle positioned so that the Luxtec® logo is properly aligned, slide the handle onto the column and center the handle about 5 inches (13cm) below the light source base plate. Tighten handle screw to hold in place.
2. Insert assembled column into the base. Seat firmly.
3. Attach the light source base onto the base plate (Figure 10) with the four (4) screws provided, using the Phillips head screwdriver provided.
4. Secure the light source to base plate by aligning the feet to the holes on the surface of the plate. Tighten the two screws on the bottom of the plate to the light source (Figure 11).

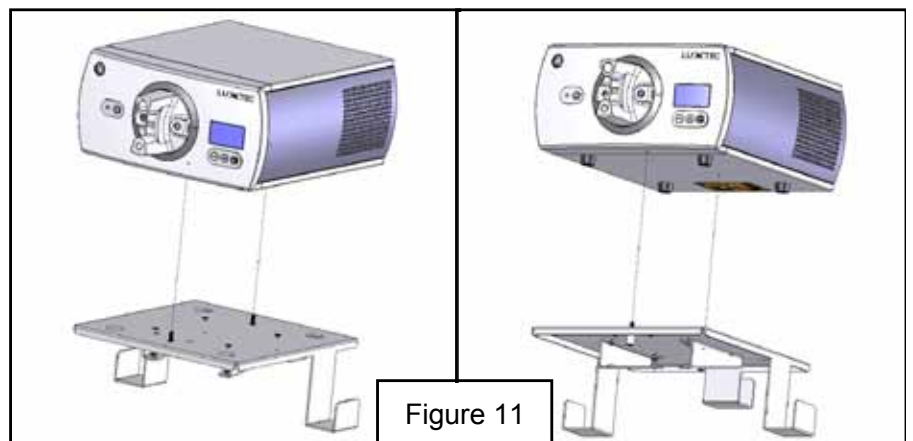

REPLACEMENT PARTS AND ACCESSORIES

To place an order, contact your local Luxtec distributor or call Luxtec Customer Service at 1-800-325-8966 (USA & Canada only) or +1-508-835-9700 to identify your local Luxtec representative.

Light Source
00MLX 300 Watt Xenon Light Source with Turret (ACMI, Wolf, Storz and Olympus)

Accessories
001320LX Xenon Lamp Module
600987 Fuse 6.3 Amp, Slow Blow
850469 Operating and Service Manual MLX light source

Optional Accessories
AX2100BIF UltraLite® Pro headlight with 9ft (275cm) premium bifurcated cable.
Mark II module and gown clips.
AX2100BIFSL UltraLite® Pro headlight with 9ft (275cm) premium bifurcated cable,
Mark II module and gown clips with short linkage.
001337 MLX Floorstand

MAINTENANCE AND CLEANING

- Allow unit to cool for at least 15 minutes prior to cleaning.
Unplug the power cord before cleaning. The light source exterior can be cleaned and disinfected using 70% isopropyl alcohol. Allow 5 minutes for alcohol to evaporate before reconnecting to power.
Use a vacuum cleaner and a soft brush to remove visible dust accumulation from fan and vent holes whenever necessary and always when replacing the lamp.

TROUBLESHOOTING

Problem	Cause	Action
No light output	Light source not turned on Bad/no lamp Attenuator closed Turret <u>mispositioned</u> Blown fuse	Turn power on Check lamp seating/replace lamp module Check position of knob on front panel Rotate turret to desired adapter fitting Replace fuse as indicated in maintenance section
Reduced light output	Cable mismatched to turret Attenuator <u>mispositioned</u> Bad lamp	Rotate turret to matching adapter fitting Check position of knob on front panel Replace lamp module
No power	Light source not plugged in Top cover not closed	Plug in light source Close and secure top cover

Fault Symbol	Cause	Action
	Lamp change (will blink after 1000 hours)	Change lamp. Module Part number 001320LX
	Fan failure	Shut off unit to reset. If it does not reset contact Luxtec for service
	Lamp overheat	Shut off system to reset. If it does not reset contact Luxtec for service
	Attenuator motor failure	Shut off system to reset. If it does not reset contact Luxtec for service

SPECIFICATIONS

Lamp Type Wattage Lamp life	Xenon Short Arc Lamp 300 Watts 1000 Hours
Light Source Dimensions Weight Power Input Fuses (2) Power Consumption AC Power Leakage Classification Electrical Safety Electromagnetic Compatibility Environment: Storage Temperature Operating Temperature Humidity Power Cord	15.4"L x 11.2"W x 5.9"H (390mm L x 285mm W x 150mm H) 12.5 lbs. (5.7 kg) 100-240VAC 50 - 60Hz± 10% 6.3A, 250VAC, 5x20 mm, Slo-Blo, IEC Standard 450 Watts (Maximum) Leakage current to chassis (with ground wire intact), less than 100 microamps Leakage current to chassis (with ground wire interrupted), less than 500 microamps Type CF, Class 1 Type A Device CSA listed, Conforms to UL 60601-1 and CSA C22.2 NO. 601.1 EN60601-1-2:2001 0°C to 50°C (32°F to 122°F) 10°C to 40°C(50°F to 104°F) 10-85% non-condensing Hospital grade

ELECTROMAGNETIC COMPATIBILITY (EMC) USER INFORMATION

WARNING: Medical Electrical Equipment needs special precautions regarding EMC and needs to be installed and put into service according to the Electromagnetic Compatibility [EMC] information provided in the accompanying documents.

WARNING: Portable and Mobile RF Communications Equipment can affect Medical Electrical Equipment.

WARNING: The equipment or system should not be used adjacent to or stacked with other equipment and that if adjacent or stacked use is necessary, the equipment or system should be observed to verify normal operation in the configuration in which it will be used.

NOTE: The EMC tables and other guidelines that are included in the Instruction Manual provide information to the customer or user that is essential in determining the suitability of the Equipment or System for the Electromagnetic Environment of use, and in managing the Electromagnetic Environment of use to permit the Equipment or System to perform its intended use without disturbing other Equipment and Systems or non-medical electrical equipment.

Table 201
Guidance and Manufacturer's Declaration – Emissions All Equipment and Systems

The MLX light source is intended for use in the electromagnetic environment specified below. The customer or user of the MLX light source should assure that it is used in such an environment.		
Emissions Test	Compliance	Electromagnetic Enforcement – guidance
RF Emissions CISPR 11	Group 1	The MLX unit uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF Emissions CISPR 11	Class B Radiated and Conducted Emissions	The MLX unit is suitable for use in all establishments including domestic, and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes. Conducted Emissions Tests Performed at both 240VAC, 50Hz and 120VAC, 60Hz
Harmonics IEC 61000-3-2	N/A	Equipment intended for Professional Use Only
Flicker IEC 61000-3-3	N/A	Equipment intended for Professional Use Only

ELECTROMAGNETIC COMPATIBILITY (EMC) USER INFORMATION

Table 202
Guidance and Manufacturer's Declaration—Immunity All Equipment and Systems

The MLX light source is intended for use in the electromagnetic environment specified below. The customer or user of the MLX light source should assure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Electrostatic Discharge (ESD) IEC 61000-4-2	±6kV contact ±8kV air	±6kV contact ±8kV air	Floors should be wood, concrete or ceramic tile. If floors are synthetic, the relative humidity should be at least 30%.
Electrical Fast Transient/burst IEC 61000-4-4	±2kV on AC Mains	±2kV on AC Mains	Mains power quality should be that of a typical commercial or hospital environment. Note - Tests Performed at both 240VAC, 50Hz and 120VAC, 60Hz
Surge IEC 61000-4-5	±1kV Differential ±2kV Common	±1kV Differential ±2kV Common	Mains power quality should be that of a typical commercial or hospital environment. Note - Tests Performed at both 240VAC, 50Hz and 120VAC, 60Hz
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	>95% Dip for 0.5 Cycle 60% Dip for 5 Cycles 30% Dip for 25 Cycles >95% Dip for 5 Seconds	>95% Dip for 0.5 Cycle 60% Dip for 5 Cycles 30% Dip for 25 Cycles >95% Dip for 5 Seconds	Mains power quality should be that of a typical commercial or hospital environment. If the user of the MLX unit requires continued operation during power mains interruptions, it is recommended that the MLX unit be powered from an uninterruptible power supply or battery. Note - Tests Performed at both 240VAC, 50Hz and 120VAC, 60Hz
Power Frequency 50/60Hz Magnetic Field IEC 61000-4-8	3A/m	3A/m	Power frequency magnetic fields should be that of a typical location in a typical commercial or hospital environment. Note - Tests Performed at both 50Hz and 60Hz

ELECTROMAGNETIC COMPATIBILITY (EMC) USER INFORMATION

Table 204

Guidance and Manufacturer's Declaration – Emissions Equipment and Systems that are NOT Life-Supporting

The MLX light source is intended for use in the electromagnetic environment specified below. The customer or user of the MLX light source unit should ensure that it is used in such an environment.

Immunity Test	IEC 60601 Test Level	Compliance Level	Electromagnetic Environment – Guidance
Conducted RF IEC 61000-4-6	3 Vrms from 150 kHz to 80 MHz	VI = 3 Vrms	Portable and mobile RF communications equipment should be separated from the MLX light source by no less than the recommended separation distances calculated/listed below: $D = (3.5 / VI) \sqrt{P}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz	EI = 3V/m	$D = (3.5 / EI) \sqrt{P}$ 80 to 800 MHz $D = (7 / EI) \sqrt{P}$ 800 MHz to 2.5 GHz Where P is the maximum power rating in watts and D is the recommended separation distance in meters. Field strengths from fixed transmitters, as determined by an electromagnetic site survey, should be less than the compliance levels (VI and EI). Interference may occur in the vicinity of equipment containing a transmitter.


Table 206

Recommended Separation Distances Between Portable and Mobile RF Communications Equipment and the MLX Equipment and Systems that are NOT Life-Supporting

The MLX light source is intended for use in the electromagnetic environment in which radiated disturbances are controlled. The customer or user of the MLX light source can help prevent electromagnetic interference by maintaining a minimum distance between portable and mobile RF Communications Equipment and the MLX light source as recommended below, according to the maximum output power of the communications equipment.

Maximum Output Power (Watts)	Recommended Separation Distances for the MLX (meters)		
	150 kHz to 80 MHz $d = 1.1667 \sqrt{P}$	80 to 800 MHz $d = 1.1667 \sqrt{P}$	800 MHz to 2.5 GHz $d = 2.3333 \sqrt{P}$
0.01	0.11667	0.11667	0.23333
0.1	0.36894	0.36894	0.73785
1	1.1667	1.1667	2.3333
10	3.6894	3.6894	7.3785
100	11.667	11.667	23.333

BLOCK DIAGRAM

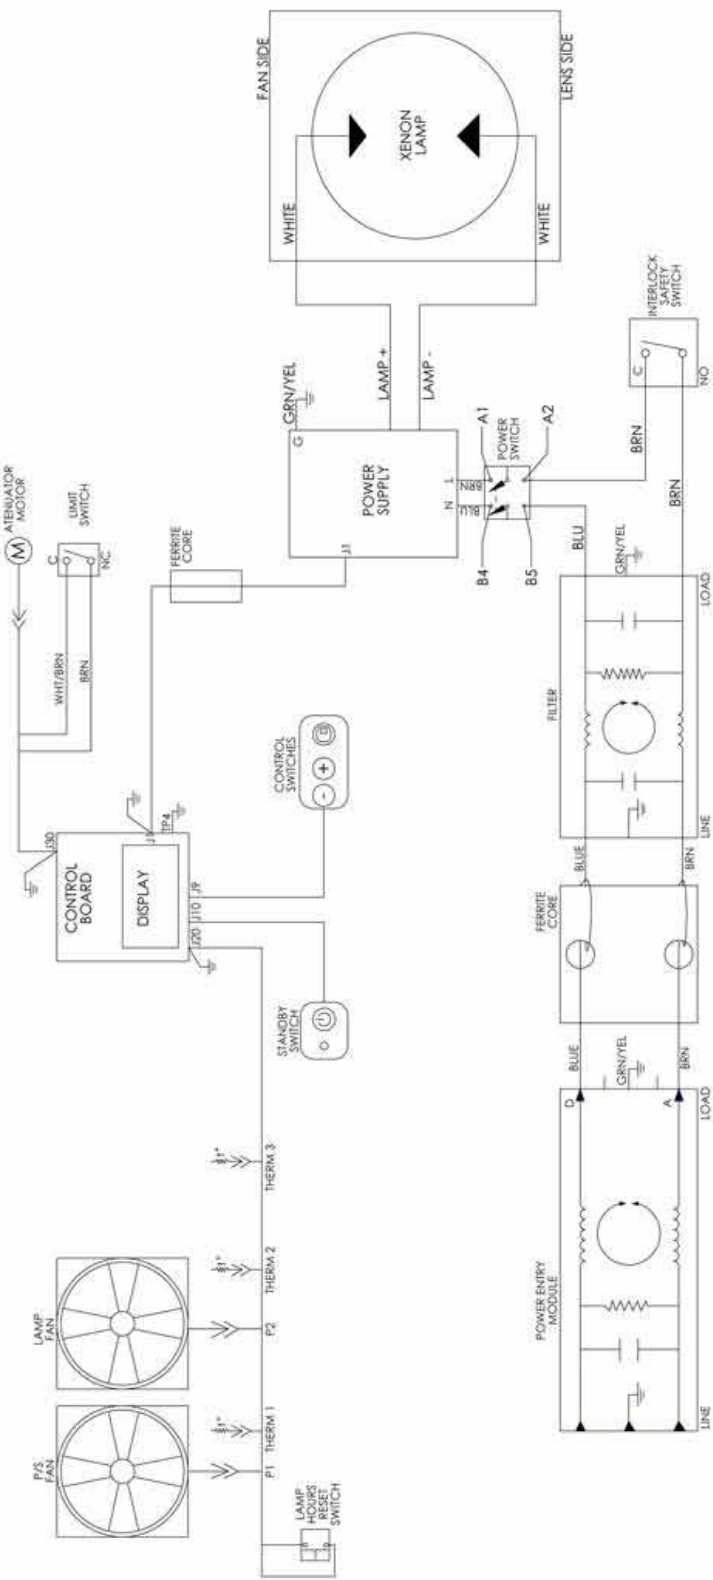

REPAIR AND RETURN INFORMATION

This device must be clean and decontaminated prior to return to Luxtec. Luxtec reserves the right to return unrepaid any equipment that is contaminated with blood or other organic material.

Warranty Service and Repair:

To obtain service under warranty or return product for repair, the customer should contact your local Luxtec representative or call Luxtec Customer Service at 1-800-325-8966 or +1-508-835-9700.

LIMITED EXPRESS WARRANTY

Luxtec warrants that the new MLX light source shall be free from defects in material and workmanship under normal use and service for a period of three (3) years from the date of shipment. Luxtec's sole and exclusive liability under the warranty shall be, at Luxtec's option, either to repair any component which fails during the warranty period due to any defect in workmanship or material F.O.B. factory if:

1. Customer promptly reports such defect to Luxtec in writing,
2. If requested by Luxtec, customer returns equipment to Luxtec with shipping charges and,
3. Upon inspection, Luxtec finds the equipment to be defective.

This warranty is contingent upon normal and proper use of the equipment. It does not cover equipment that has been modified with non-Luxtec parts without the written approval of Luxtec, subjected to unusual physical or electrical stress, or damaged during shipment. This warranty is non-transferable unless authorized in writing by Luxtec.

Luxtec reserves the right to make design changes on its products without liability to incorporate said change in Luxtec products previously designed or sold.

Upon receipt of the product, it should be carefully inspected. If any defect is discovered, notification must be given immediately to the manufacturer or authorized distributor.



www.Integra-Surgical.com

The Integra wave logo and Integra Surgical are trademarks of Integra LifeSciences Corporation.
Luxtec and UltraLite are registered trademark of Integra LifeSciences Corporation or its subsidiaries.
Copyright © 2010 Integra LifeSciences Corporation. All rights reserved.

THE INSTRUMENT PEOPLE

LUXTEC OMNI-TRACT JATE PADGETT REDMOND